

36 materials; 6 corridor lengths; fitting heights starting at 13mm.

KODAK Unique Progressives feature a backside design for enhanced optical performance.

Available in six corridor lengths: 13mm, 14mm, 15mm, 16mm, 17mm and 18mm. KODAK Unique Lenses are not available with Rx prism.


Add Range: +0.75 to +3.50 in .25 D steps	Lens Material KODAK Unique Lenses only available coated.	Sphere Range	Cylinder Range to a -4.00	Maximum Cutout	Index of Refraction	Abbe Value	Specific Gravity
Standard Index	Standard Resin	+4.00 to -8.00	limited to a combined sph/cyl power of -8.00	70mm	1.499	58	1.32 gm/cm ³
	*Trivex®	+4.50 to -10.00	limited to a combined sph/cyl power of -10.00	65mm	1.53	44	1.11 gm/cm ³
Thinner, Lighter Lenses	*PolyClear®	+5.00 to -10.00	limited to a combined sph/cyl power of -10.00	73mm	1.586	28	1.20 gm/cm ³
	EvoClear® 1.56	+5.00 to -10.00	limited to a combined sph/cyl power of -10.00	69mm	1.557	36	1.24 gm/cm ³
	*TLX 1.6™	+6.00 to -11.00	limited to a combined sph/cyl power of -11.00	70mm	1.594	42	1.30gm/cm ³
	*1.67 High Index	+6.00 to -12.00	limited to a combined sph/cyl power of -12.00	70mm	1.666	32	1.34 gm/cm ³
	1.74 High Index	+9.00 to -13.25	limited to a combined sph/cyl power of -13.25	70mm	1.738	33	1.47 gm/cm ³
Polarized	SA PolarShades® Standard Resin <i>Gray and Brown</i>	+4.00 to -6.75	limited to a combined sph/cyl power of -6.75	73mm	1.499	58	1.32 gm/cm ³
	*SA PolarShades 1.60 <i>Gray and Brown</i>	+5.75 to -11.00	limited to a combined sph/cyl power of -11.00	70mm	1.60	42	1.30 gm/cm ³
	*SA PolarShades 1.67 <i>Gray and Brown</i>	+7.50 to -13.00	limited to a combined sph/cyl power of -13.00	70mm	1.666	32	1.34 gm/cm ³
	*SA PolarShades Polycarbonate <i>Gray and Brown</i>	+5.00 to -11.00	limited to a combined sph/cyl power of -11.00	70mm	1.586	28	1.20 gm/cm ³
Photochromic/ Polarized	Drivewear®	+4.00 to -8.00	limited to a combined sph/cyl power of -8.00	69mm	1.50	57	1.27 gm/cm ³
Photochromic	*InstaShades® 1.50 <i>Gray</i>	+4.00 to -8.00	limited to a combined sph/cyl power of -8.00	69mm	1.508	52	1.19 gm/cm ³
	*KODAK InstaShades PolyClear® <i>Gray and Brown</i>	+5.00 to -10.00	limited to a combined sph/cyl power of -10.00	69mm	1.586	28	1.20 gm/cm ³
	KODAK InstaShades EvoClear® 1.6 <i>Gray and Brown</i>	+6.00 to -11.00	limited to a combined sph/cyl power of -11.00	67mm	1.594	32	1.34 gm/cm ³
	KODAK InstaShades EvoClear 1.56 <i>Gray and Brown</i>	+5.00 to -10.00	limited to a combined sph/cyl power of -10.00	67mm	1.557	36	1.21 gm/cm ³
	Corning® SunSensors® 1.56 <i>Gray and Brown</i>	+5.00 to -10.00	limited to a combined sph/cyl power of -10.00	69mm	1.555	38	1.17 gm/cm ³
	*Life Rx™ Polycarbonate <i>Gray and Brown</i>	+5.00 to -10.00	limited to a combined sph/cyl power of -10.00	70mm	1.586	28	1.20 gm/cm ³
	Transitions® 1.50 <i>Gray and Brown</i>	+4.00 to -8.00	limited to a combined sph/cyl power of -8.00	71mm	1.497	57	1.27 gm/cm ³
	*Transitions Polycarbonate <i>Gray and Brown</i>	+5.00 to -10.00	limited to a combined sph/cyl power of -10.00	70mm	1.586	28	1.20 gm/cm ³
	*Transitions Trivex® <i>Gray and Brown</i>	+4.50 to -10.00	limited to a combined sph/cyl power of -10.00	65mm	1.53	44	1.11 gm/cm ³
	*Transitions 1.60 <i>Gray and Brown</i>	+6.00 to -11.00	limited to a combined sph/cyl power of -11.00	60mm	1.596	42	1.30gm/cm ³
	*Transitions 1.67 <i>Gray</i>	+6.00 to -12.00	limited to a combined sph/cyl power of -12.00	69mm	1.666	32	1.34 gm/cm ³
	* Recommended for drill mount frames.						

Dispensing Instructions

- Select the frame.** The frame should accommodate a minimum 13mm fitting height to the bottom of the eyewire and 10mm to the top. Adjust the frame for comfort and accuracy before taking measurements. Adjustable nose pads are recommended. Set the pantoscopic angle to 10-12°. Frame should have a slight face form.
- PD and Fitting Height.** Measure monocular fitting height by marking each demo lens at the pupil centers with a felt tip pen. Measure monocular PD using a pupilometer or by using the fitting height marks. To translate lens markings into measurements, place the frame on the center of the triangle, ensuring the marks on the lens are on the zero (0) line. Using the chart, record the monocular PD and monocular vertical heights.
- Frame verification.** Line up the pupillary mark on the demo lens with the cross on the chart. Verify that the distance and near zones are within the blue circle and that the eyewire is within the cutout diameter. This will ensure the minimum fitting height and cutout specifications are met. Confirm that the lens cutout is compatible with the material type you are specifying.
- Include this information.** Make sure you include the following information in your KODAK Unique Progressive lab order. These pieces of information are critical to the correct customization and optimization of the design to the frame size and shape.
 - Monocular PD measurements
 - Monocular fitting height measurements
 - Manually traced right eyewire drawing
 - Frame A, B, and DBL dimensions
 - Frame brand, model, and eyeseize


Note: KODAK Unique Progressives cannot be supplied unless items "a" through "d" above are provided.
- Dispensing.** Confirm the monocular PD and fitting height. Verify the lens R on the lensometer. Confirm the fit on the patient by verifying that the fitting cross is properly positioned over the pupil. Adjust the frame as necessary.
- Teach proper viewing.** Demonstrate the different viewing areas and appropriate head and eye movement.

PD and Fitting Height Chart

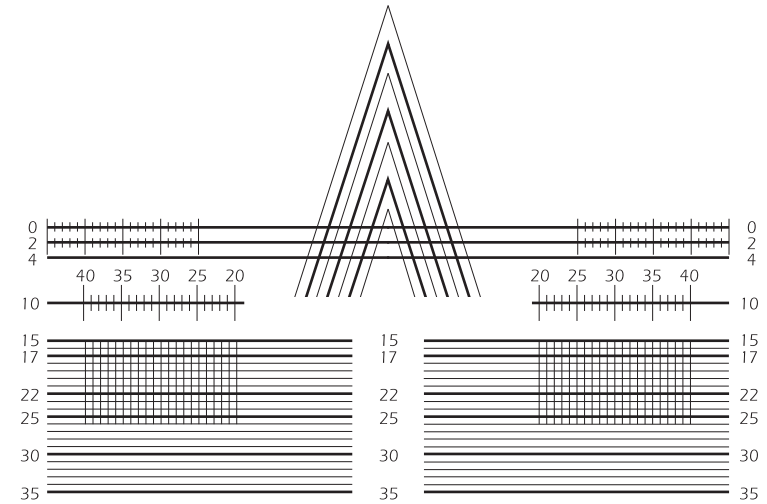

IMPORTANT If the entire lens is within the yellow area, it will be too small to be surfaced. You should recommend a different frame.

Frame Verification Chart (LEFT)

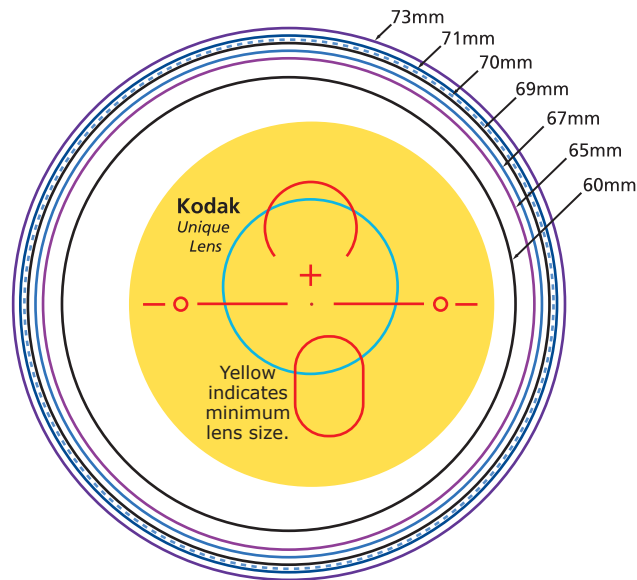

Frame Verification Chart (RIGHT)

